

DONJOY® VELOCITY®+ ANKLE

patientapplication

BEFORE APPLYING THE BRACE, PLEASE READ THESE INSTRUCTIONS COMPLETELY AND CAREFULLY. CORRECT APPLICATION IS VITAL TO PROPER FUNCTIONALITY OF THE BRACE.


INTENDED USE/INDICATIONS:

The Donjoy Velocity®+ Ankle is designed to provide support to the ankle and relief pain following injuries such as ankle sprains and chronic ankle instabilities. Soft-good/semi-rigid designed to restrict motion through elastic or semi-rigid construction.

APPLICATION OF THE BRACE:


1.

Unfasten and loosen all straps. Place ankle in the brace and position at 90°.

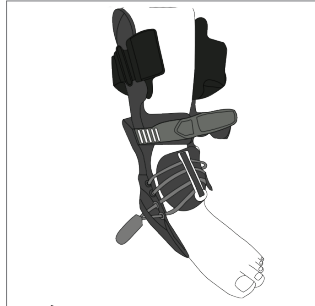


5.

Pull, wrap, and lock both calf ratchet straps snugly into place without impairing circulation.

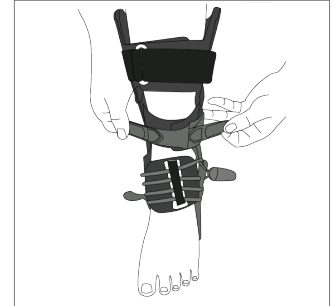


2.

Wrap and secure calf liner.

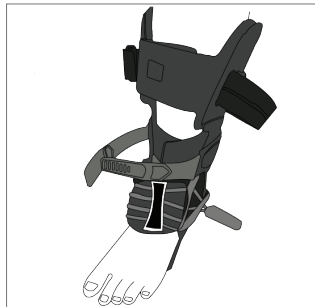


6.

Align tongue with the center of the forefoot MS and ES versions only.

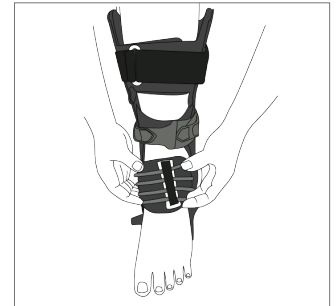


3.

Tighten and fasten the proximal, circumferential extension cuff hook and loop strap.

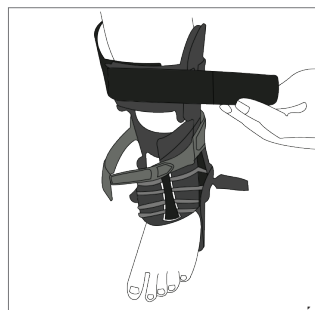


7.

Pull and wrap ankle strap(s) snugly into place without impairing circulation.

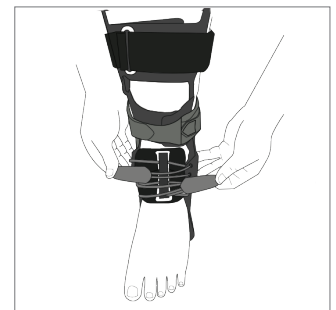

4.

Insert calf ratchet strap end through opening on the opposite calf ratchet strap.

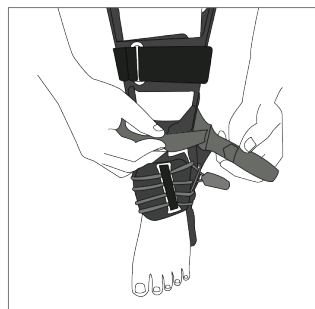

Note


The lace guide on the tongue may be adjusted and the Achilles pad may be trimmed to fit individual variations in leg, ankle joint, and foot shape.

PATENTED
FOR SINGLE PATIENT USE ONLY.

OPTIONAL REMOVAL OF PROXIMAL EXTENSION CUFF:


8.

With the brace removed from the leg, disengage the calf liner from the proximal extension cuff.

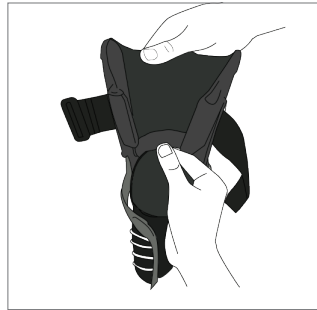


9.

Next, detach the proximal extension cuff from the posterior, inside aspect of the rigid calf support.

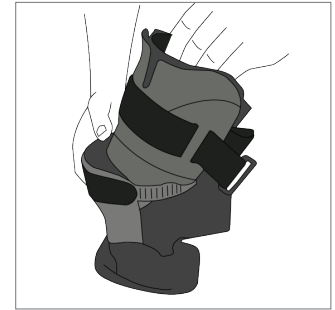

10.

Reattach the calf liner to the rigid calf support.

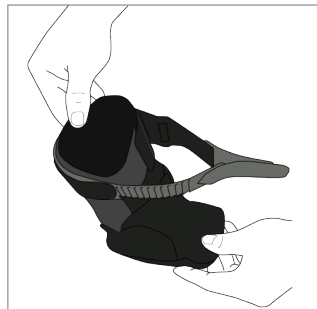

USE AND CARE:

To clean liners, hand wash in cold water using mild soap. Air dry.

Note: If not rinsed thoroughly, residual soap may cause irritation and deteriorate material.

WARNINGS AND PRECAUTIONS:

1. Do not use over open wounds.
2. If pain, swelling, changes in sensation or other unusual reactions occur while using this product, you should contact your doctor immediately.
3. Do not attempt to heat mould any component other than the foot plate.
4. Do not use an oven, boiling water, or any heat source other than a heat gun. Refer to heat gun manufacturer's instructions for use for additional warnings and precautions.
5. Do not heat foot plate to more than 300°F as melting may occur.
6. Do not use this device if it was damaged and/or package has been opened.
7. If you develop an allergic reaction and/or experience itchy, red skin after coming into contact with any part of this device, please stop using it and contact your healthcare professional immediately.

NOTE: Contact manufacturer and competent authority in case of a serious incident arising due to usage of this device.

Next appointment:

Date: _____

Time: _____

Notes: _____



DJO, LLC
 T 800.336.6569 F 800.936.6569
 5919 Sea Otter Place, Suite 200 | Carlsbad, CA 92010 | U.S.A.
DJOglobal.com

COPYRIGHT © DJO, LLC 2024

MKTIS00-13332 Rev A

Individual results may vary. Neither DJO, LLC nor any of the Enovis companies dispense medical advice. The contents of this document do not constitute medical, legal, or any other type of professional advice. Rather, please consult your healthcare professional for information on the courses of treatment, if any, which may be appropriate for you.